

## Quiz: ICD

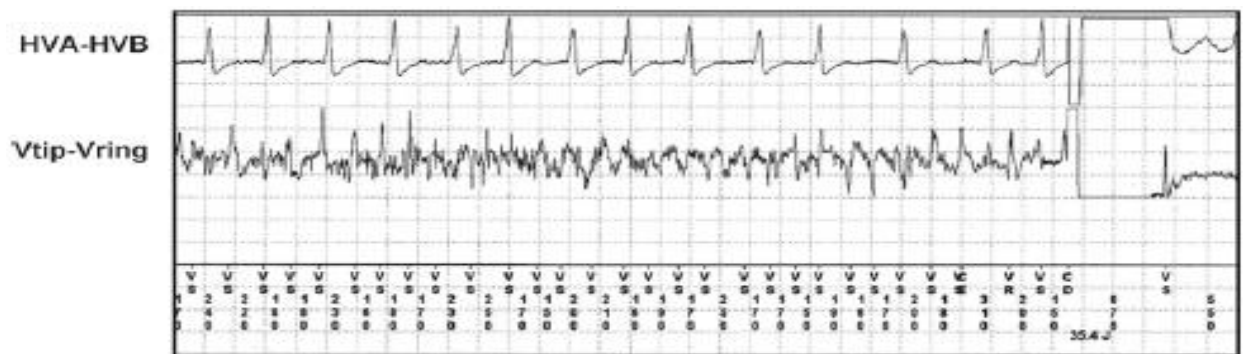


Figure 1. Stored electrogram

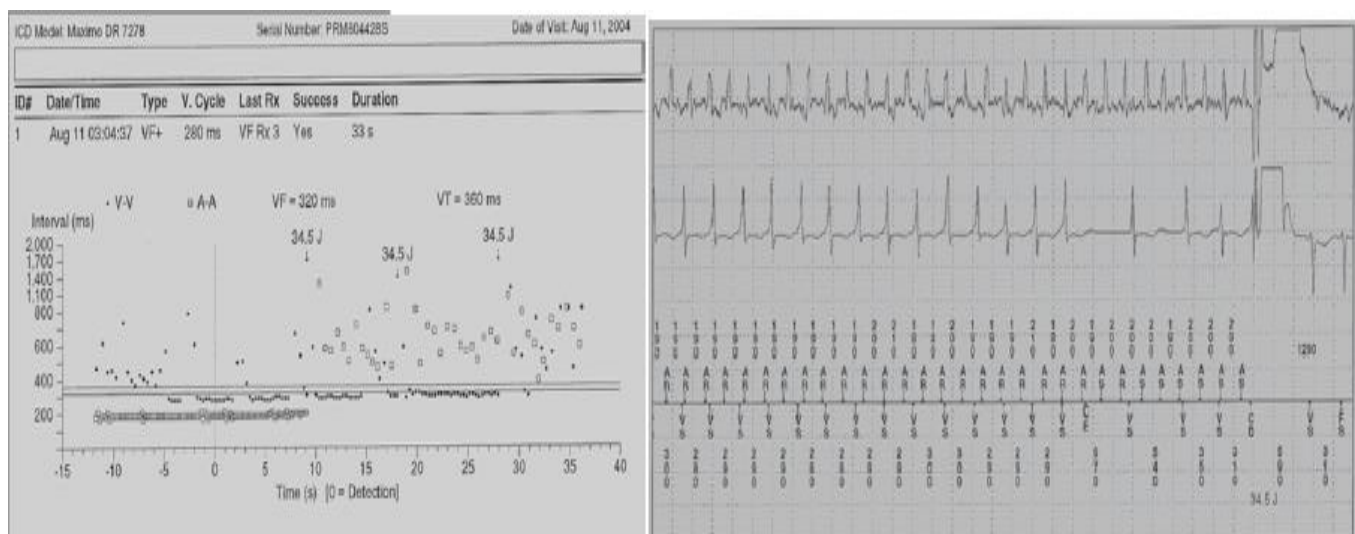


Figure 2. Stored electrogram

Consider these cases. What happened and what reasons led to this?

- A. Inappropriate ICD discharges: noise on the RV electrode on Fig.1 Rapid atrial fibrillation on Fig.2
- B. Inappropriate ICD discharges: T wave oversensing on Fig.1 Rapid atrial flutter on Fig.2
- C. Appropriate ICD discharges: Ventricular fibrillation on Fig.1 Rapid ventricular tachycardia on Fig.2
- D. Inappropriate ICD discharges: T wave oversensing on Fig.1 Pacemaker-mediated tachycardia on Fig.2

Ayan Abdrakhmanov, Zhandos Esilbayev  
 Department of Interventional  
 Arrhythmology  
 National Research Cardiac Surgery  
 Center  
 Nur-Sultan, Kazakhstan

**Peer-review:** Internal  
**Conflict of interest:** None to declare

**Authorship:** A.A. and Z.E. equally  
 contributed to preparation of quiz

**Acknowledgement and funding:** None to  
 declare

**Address for Correspondence:** Ayan Abdrakhmanov, Department of Interventional Arrhythmology,  
 National Research Cardiac Surgery Center, Nur-Sultan, Kazakhstan, Email: [ayan-3@mail.ru](mailto:ayan-3@mail.ru)

**Received** 24.01.2019 **Accepted:** 25.01.2019

**Copyright** © 2019 Heart, Vessels and Transplantation

doi: 10.24969/hvt.2019.